

ETHYLENE OXIDE

Method no.: 30

Matrix: Air

Target concentration: 1.0 ppm (1.8 mg/m³)

Procedure: Samples are collected on two charcoal tubes in series and desorbed with a benzene/CS₂ (99:1) desorption solution. The samples are derivatized with HBr and treated with sodium carbonate. Analysis is done by gas chromatography with an electron capture detector.

Recommended air volume and sampling rate: 1 L and 0.05 L/min

Detection limit of the overall procedure: 13.3 ppb (24.0 µg/m³)

Reliable quantitation limit: 52.2 ppb (94.0 µg/m³)

Standard error of estimate: 6.59%
(Figure 4.6.2.)

Special requirements: Samples must be analyzed within 15 days of sampling date. (Figures 4.6.1. and 4.6.2.)

Status of method: Evaluated method. This method has been subjected to the established evaluation procedures of the Organic Methods Evaluation Branch.

Date: August 1981

Chemist: Wayne D. Potter

Organic Solvents Branch
OSHA Analytical Laboratory
Salt Lake City, Utah

1. General Discussion

1.1. Background

1.1.1. History

Ethylene oxide air samples analyzed at the OSHA Laboratory have normally been collected on activated charcoal and desorbed with carbon disulfide (CS₂). The analysis is performed with a gas chromatograph equipped with a flame ionization detector (FID), as described in NIOSH Method S286 (Ref. 5.1). This method is based on a PEL of 50 ppm and has a detection limit of about 1 ppm.

Recent studies (Section 1.1.2.) have prompted the need for a method to detect and quantitate ethylene oxide at very low concentrations.

Several attempts were made to form an ultraviolet (UV) sensitive derivative with ethylene oxide for analysis with HPLC. Among those tested that gave no detectable product were: p-anisidine, methylimidazole, aniline, and 2,3,6-trichlorobenzoic acid. Each was tested with catalysts such as triethylamine, aluminum chloride, methylene chloride and sulfuric acid, but no detectable derivative was produced.

The next derivatization attempt was to react ethylene oxide with HBr to form 2-bromoethanol. This reaction was successful. An electron capture detector (ECD) gave a very good response for 2-bromoethanol due to the presence of bromine. The use of CS₂ as the desorbing solvent gave too large of a response and masked the 2-bromoethanol. Several other solvents were tested for both their response on the ECD and their ability to desorb ethylene oxide from the charcoal. Among those tested were toluene, xylene, ethyl benzene, hexane, cyclohexane and benzene. Benzene was the only solvent tested that gave a suitable response on the ECD and a high desorption. It was found that the desorption efficiency was improved by using a benzene/CS₂ (99:1) desorption solution. The addition of CS₂ to other tested desorption solvents did not significantly improve the recovery. SKC Lot 120 was used in all tests done with activated charcoal.

1.1.2. Toxic effects (This section is for information only and should not be taken as the basis for OSHA policy.)

Ethylene oxide has recently been found to cause an increase in incidences of mononuclear cell leukemia and peritoneal mesothelioma in rats. The rats were exposed to ethylene oxide vapor concentrations of 10, 33 and 100 ppm for 6 h a day, 5 days a week, for up to two years. Post-mortem examinations were made on all animals that died or

were killed when moribund, and at scheduled intervals of 6, 12, 18, 24 and 25 months. Female rats exposed to 100 ppm ethylene oxide had a significant increase in mono-nuclear cell leukemia and female rats exposed to 33 and 100 ppm also showed a dose response for leukemia incidences. In male rats, the incidences of peritoneal mesothelioma was found to be treatment-related at exposures of 33 and 100 ppm (Ref. 5.3.).

The ability of a chemical to serve as an alkylating agent and to cause mutations in a variety of biological test systems is widely accepted as an indicator that the chemical may have carcinogenic potential. Both alkylation and mutagenicity have been demonstrated for ethylene oxide (Ref. 5.3.).

According to NIOSH, epidemiologic investigations for cancer in humans are too limited to be cited as definitive evidence of an excess risk of cancer resulting from ethylene oxide exposure, but their findings should be considered evidence that an excess risk of cancer may exist for those ethylene oxide workers studied. NIOSH recommends that ethylene oxide be regarded in the workplace as a potential occupational carcinogen (Ref. 5.3.).

Ethylene oxide may be described as a central depressant, irritant, and protoplasmic poison. Contact with even a dilute solution may cause irritation and necrosis of the eyes, and irritation, blistering, edema, and necrosis of the skin. Excessive exposure to the vapor may cause irritation of the eyes, respiratory tract and lungs, and central depression. Nausea and vomiting are usually delayed and may be followed by convulsive seizure and profound weakness of the extremities, and secondary infection of the lungs (Ref. 5.2.).

1.1.3. Potential workplace exposure

Industries and activities which use a small portion of the annual production of ethylene oxide, such as health care, are responsible for high occupational exposures to many workers. In 1977, NIOSH estimated 75,000 health care workers in sterilization areas were potentially exposed to ethylene oxide. It is also used in small volumes as a fumigant or sterilant in the following areas: medical products manufacturing, libraries, museums, research laboratories, bookkeeping, spices, seasonings, black walnut meat fumigation, dairy packaging, cosmetics manufacturing, animal and plant quarantine service at ports of entry, transportation vehicles fumigation, clothing, furs, and furniture fumigation. The large volume uses of ethylene oxide such as in the production of ethylene glycol, surface-active agents, glycol ethers and ethanol amines may

not involve serious occupational exposure since process equipment generally consists of tightly closed and highly automated systems (Ref. 5.3.).

1.1.4. Physical properties (Refs. 5.4.-5.6.)

synonyms:	oxirane; dimethylene oxide; oxane; 1,2-epoxy ethane; C ₂ H ₄ O; ETO
molecular weight:	44.06
boiling point:	10.7°C
melting point:	-111°C
description:	colorless, flammable gas
vapor pressure:	1095 mm Hg at 20°C
odor:	ether-like odor
lower explosive limit:	3.0% (by volume)
flash point (TOC):	below 0°F
molecular structure:	$\begin{array}{c} \text{H}_2\text{C} - \text{CH}_2 \\ \quad \backslash \ / \\ \quad \quad \text{O} \end{array}$

1.2. Limit defining parameters

1.2.1. Detection limit of the analytical procedure

The detection limit of the analytical procedure is 12.0 pg of ethylene oxide per injection. This is the amount of analyte which will give a peak whose height is five times the height of the baseline noise. (Section 4.1.)

1.2.2. Detection limit of the overall procedure

The detection limit of the overall procedure is 24.0 ng of ethylene oxide per sample (13.3 ppb or 24.0 µg/m³). This is the amount of analyte spiked on the sampling device which allows recovery of an amount of analyte equivalent to the detection limit of the analytical procedure (Figure 4.2.1.).

1.2.3. Reliable quantitation limit

The reliable quantitation limit is 94.0 ng of ethylene oxide per sample (52.2 ppb or 94.0 µg/m³). This is the smallest amount of analyte which can be quantitated within the requirements of 75% recovery and 95% confidence limits of ±25%. (Figure 4.2.2.)

The reliable quantitation limit and detection limits reported in the method are based upon optimization of the instrument for the smallest possible amount of analyte. When the target concentration of an analyte is exceptionally higher than these limits, they may not be attainable at the routine operating parameters.

1.2.4. Sensitivity

The sensitivity of the analytical procedure over a concentration range representing 0.5 to 2 times the target concentration based on the recommended air volume is 34,105 area units per $\mu\text{g/mL}$. The sensitivity is determined by the slope of the calibration curve. (Section 4.3.) The sensitivity will vary somewhat with the particular instrument used in the analysis.

1.2.5. Recovery

The recovery of analyte from the collection medium must be 75% or greater. The average recovery from spiked samples over the range of 0.5 to 2 times the target concentration is 88.0%. (Section 4.4.) At lower concentrations the recovery appears to be nonlinear. (Figure 4.2.2.)

1.2.6. Precision (analytical method only)

The pooled coefficient of variation obtained from replicate determination of analytical standards at 0.5, 1 and 2 times the target concentration is 0.036. (Section 4.5.)

1.2.7. Precision (overall procedure)

The overall procedure must provide results at the target concentration that are $\pm 25\%$ or better at the 95% confidence level. The precision at the 95% confidence level for the 15-day storage test is $\pm 12.9\%$ (Section 4.6. and Figure 4.6.2.). This includes an additional $\pm 5\%$ for sampling error.

1.3. Advantages

1.3.1. The sampling procedure is convenient.

1.3.2. The analytical procedure is very sensitive and reproducible.

1.3.3. Reanalysis of samples is possible.

1.3.4. Samples are stable for at least 15 days at room temperature.

1.3.5. Interferences are reduced by the longer GC retention time of the new derivative.

1.4. Disadvantages

1.4.1. Two tubes in series must be used because of possible breakthrough.

- 1.4.2. The precision of the sampling rate may be limited by the reproducibility of the pressure drop across the tubes. The pumps are usually calibrated for one tube only.
- 1.4.3. The use of benzene as the desorption solvent increases the hazards of analysis because of the potential carcinogenic effects of benzene.
- 1.4.4. After repeated injections there can be a build-up of residue formed on the electron capture detector which decreases sensitivity.
- 1.4.5. Recovery from the charcoal tubes appears to be nonlinear at low concentrations.

2. Sampling Procedure

2.1. Apparatus

- 2.1.1. A calibrated personal sampling pump whose flow can be determined with $\pm 5\%$ of the recommended flow.
- 2.1.2. SKC Lot 120 Charcoal tubes (catalog no. 226-01): glass tube with both ends flame sealed, 70 mm x 6-mm o.d. x 4-mm i.d., containing 2 sections of coconut shell charcoal separated by a 2-mm portion of urethane foam. The adsorbing section contains 100 mg of charcoal, the backup section 50 mg. A 3-mm portion of urethane foam is placed between the outlet end of the tube and the backup section. A plug of silylated glass wool is placed in front of the adsorbing section.

2.2. Reagents

None required

2.3. Sampling technique

- 2.3.1. Immediately before sampling, break the ends of the charcoal tubes. All tubes must be from the same lot.
- 2.3.2. Connect two tubes in series to the sampling pump with a short section of flexible tubing. A minimum amount of tubing is used to connect the two sampling tubes together. The tube closer to the pump is used as a backup. This tube should be identified as the backup tube.
- 2.3.3. The tubes should be placed in a vertical position during sampling to minimize channeling.
- 2.3.4. Air being sampled should not pass through any hose or tubing before entering the charcoal tubes.

- 2.3.5. Seal the charcoal tubes with plastic caps immediately after sampling.
- 2.3.6. With each batch of samples, submit at least one blank tube from the same lot used for samples. This tube should be subjected to exactly the same handling as the samples (break, seal, transport) except that no air is drawn through it.
- 2.3.7. Transport the samples (and corresponding paperwork) to the lab for analysis.
- 2.3.8. If bulk samples are submitted for analysis, they should be transported in glass containers with Teflon-lined caps. These samples must be mailed separately from the container used for the charcoal tubes.

2.4. Breakthrough

The breakthrough (5% breakthrough) volume for a 3.0 mg/m³ ethylene oxide sample stream at approximately 85% relative humidity, 22°C and 633 mm Hg is 2.6 L sampled at 0.05 L/min. This is equivalent to 7.8 µg of ethylene oxide. Upon saturation of the tube it appeared that the water may be displacing ethylene oxide during sampling as shown in Figure 4.7.

2.5. Desorption efficiency

- 2.5.1. The desorption efficiency, determined from charcoal tubes spiked by liquid injection, averaged 88.0% from 0.5 to 2.0 times the target concentration for a 1-L air sample (Section 4.4.). At lower levels it appears that the desorption efficiency is nonlinear (Section 4.2.).
- 2.5.2. The desorption efficiency may vary from one laboratory to another and also from one lot of charcoal to another. Thus, it is necessary to determine the desorption efficiency for a particular lot of charcoal.

2.6. Recommended air volume and sampling rate

- 2.6.1. The recommended air volume is 1.0 L.
- 2.6.2. The recommended maximum sampling rate is 0.05 L/min.

2.7. Interferences

- 2.7.1. Ethylene glycol and Freon 12 at target concentration levels did not interfere with the collection of ethylene oxide.
- 2.7.2. Suspected interferences should be listed on the sample data sheets.

2.7.3. The relative humidity may affect the sampling procedure.

2.8. Safety precautions

2.8.1. Attach the sampling equipment to the employee so that it does not interfere with work performance.

2.8.2. Wear safety glasses when breaking the ends of the sampling tubes.

2.8.3. If possible, place the sampling tubes in a holder so the sharp end is not exposed while sampling.

3. Analytical Procedure

3.1. Apparatus

3.1.1. Gas chromatograph equipped with a linearized electron capture detector.

3.1.2. GC column capable of separating the derivative of ethylene oxide (2-bromoethanol) from any interferences, benzene and CS₂. The column used for validation studies was: 10 ft x 1/8 in., stainless steel, 20% SP-2100, 0.1% Carbowax 1500 coated on 100/120 Supelcoport.

3.1.3. An electronic integrator or some other suitable method of measuring peak areas.

3.1.4. Two-milliliter vials with Teflon-lined caps.

3.1.5. Gas-tight syringe, 500- μ L or other convenient sizes for preparing standards.

3.1.6. Microliter syringes, 10- μ L or other convenient sizes for diluting standards and 1- μ L for sample injections.

3.1.7. Pipets for dispensing the benzene/CS₂ (99:1) desorption solution. A Glenco 1-mL dispenser is adequate and convenient.

3.1.8. Volumetric flasks, 5-mL and other convenient sizes for preparing standards.

3.1.9. Disposable Pasteur pipets.

3.2. Reagents

3.2.1. Benzene, reagent grade.

3.2.2. Carbon disulfide, reagent grade.

3.2.3. Desorbing reagent, benzene/CS₂ (99:1) (v/v).

- 3.2.4. Ethylene oxide, 99.7% pure.
- 3.2.5. Hydrobromic acid, 48%, reagent grade.
- 3.2.6. Sodium carbonate, anhydrous, reagent grade.

3.3. Standard preparation

- 3.3.1. Standards are prepared by injecting pure ethylene oxide gas into the desorbing reagent.
- 3.3.2. A range of standards are prepared to make a calibration curve. A concentration of 1.0 μ L of ethylene oxide gas per 1 mL of desorbing reagent is equivalent to 1.0 ppm air concentration (all gas volumes at 25°C and 760 mm) for the recommended 1-L air sample.
- 3.3.3. One drop of HBr per milliliter of standard is added and mixed well.
- 3.3.4. About 0.15 g of sodium carbonate is carefully added for each drop of HBr. (A small gas-producing reaction will occur).

3.4. Sample preparation

- 3.4.1. The front and back sections of each sample are transferred to separate 2-mL vials.
- 3.4.2. Each sample is desorbed with 1.0 mL of desorbing reagent.
- 3.4.3. The vials are sealed immediately and allowed to desorb for 1 h with occasional shaking.
- 3.4.4. Desorbing reagent is drawn off the charcoal with a disposable pipet and put into clean 2-mL vials.
- 3.4.5. One drop of HBr is added to each vial. The vials are resealed and HBr is mixed well with the desorbing reagent.
- 3.4.6. About 0.15 g of sodium carbonate is carefully added to each vial. The vials are again resealed and mixed well.

3.5. Analysis

3.5.1. GC conditions

nitrogen flow rate: 10 mL/min
injector temperature: 250°C
detector temperature: 300°C
column temperature: 100°C
injection size: 0.8 μ L
elution time: 3.9 min
chromatogram: Figure 4.8.

3.5.2. Peak areas are measured by an integrator or other suitable means.

3.5.3. A calibration curve is prepared by plotting concentration of ethylene oxide (in $\mu\text{g/mL}$) versus area units.

3.6. Interferences

3.6.1. Any compound having the same retention time as 2-bromoethanol is a potential interference. Possible interferences should be listed on the sample data sheets.

3.6.2. GC parameters may be changed to circumvent interferences.

3.6.3. There are usually trace contaminants in benzene. These contaminants, however, presented no interference problems.

3.6.4. Retention time data on a single column is not considered proof of chemical identity. Samples over the PEL should be confirmed by GC/MS or other suitable means.

3.7. Calculations

3.7.1. The concentration in $\mu\text{g/mL}$ for a sample is determined by comparing the peak area of the 2-bromoethanol to the calibration curve, which had been prepared from analytical standards.

3.7.2. The amount of analyte in each sample is corrected for desorption efficiency by use of a desorption curve (Figure 4.2.2.).

3.7.3. Analytical results (A) from the two tubes that compose a particular air sample are added together.

3.7.4. The concentration for a sample is calculated by the following equation:

$$\text{ETO, mg/m}^3 = (\text{A})(\text{B})/\text{C}$$

where A = $\mu\text{g/mL}$

B = desorption volume in milliliters

C = air volume in liters

3.7.5. To convert mg/m^3 to parts per million (ppm) the following relationship is used:

$$\text{ETO, ppm} = (\text{mg/m}^3)(24.46)/44.05$$

where mg/m^3 = results from 3.7.4.

24.46 = molar volume at 25°C and 760 mm Hg

44.05 = molecular weight of ETO

3.8. Safety precautions

- 3.8.1. Ethylene oxide and benzene are potential carcinogens and care must be exercised when working with these compounds.
- 3.8.2. All work done with the solvents (preparation of standards, desorption of samples, etc.) should be done in a hood.
- 3.8.3. Avoid skin contact with all of the solvents.
- 3.8.4. Wear safety glasses at all times.
- 3.8.5. Avoid skin contact with HBr because it is highly toxic and a strong irritant to eyes and skin.

4. Backup Data

4.1. Detection limit

The detection limit was determined by injecting 0.8 μL of a 0.015 $\mu\text{g/mL}$ standard of ethylene oxide into benzene/ CS_2 (99:1). The detection limit of the analytical procedure is taken to be 12 pg per injection. This is equivalent to 8.3 ppb (15.0 $\mu\text{g/m}^3$) for the recommended air volume. A chromatogram of the analytical detection limit is shown in Figure 4.1.

4.2. Desorption efficiency

Ethylene oxide was spiked onto charcoal tubes and the following recovery data was obtained. The detection limit for the overall procedure is shown in Figure 4.2.1. The recovery curve is shown in Figure 4.2.2.

Table 4.2.
Desorption Efficiency

amount spiked (μg)	amount recovered (μg)	% recovery
4.5	4.32	96.0
3.0	2.61	87.0
2.25	2.025	90.0
1.5	1.365	91.0
1.5	1.38	92.0
0.75	0.6525	87.0
0.375	0.315	84.0
0.375	0.312	83.2
0.1875	0.151	80.5
0.094	0.070	74.5

At lower amounts the recovery appears to be nonlinear.

4.3. Sensitivity

The following data, resulting from the multiple injections of three analytical standards, were used to determine the calibration curve. The calibration curve is shown in Figure 4.3.

Table 3.3.
Sensitivity Data

x target conc. µg/mL	0.5x	1x	2x
area counts	30904	59567	111778
	30987	62914	106016
	32555	58578	106122
	32242	57173	109716
\bar{X}	31672	59558	108408

4.4. Recovery

The recovery was determined by spiking sets of lot 120 charcoal tubes with ethylene oxide and desorbing them with benzene/CS₂ (99:1). Recoveries were determined at 0.5, 1.0, and 2.0 times the target concentration (1 ppm) for the recommended air volume.

Table 4.4.
Recovery

x target conc.	0.5x	1x	2x
% recovered	88.7	95.0	91.7
(desorption	83.8	95.0	87.3
efficiency)	84.2	91.0	86.0
	88.0	91.0	83.0
	88.0	86.0	
		85.0	
\bar{X}	86.5	90.5	87.0
weighted average = 88.2			

4.5. Precision of the analytical procedure

The following data was used to determine the precision of the analytical method:

Table 4.5.
Precision of the Analytical Procedure

x target conc. µg/mL	0.5x 0.75	1x 1.5	2x 3.0
µg/mL found	0.7421 0.7441 0.7831 0.7753	1.4899 1.5826 1.4628 1.4244	3.1184 3.0447 2.9149 2.9185
\bar{X}	0.7612	1.4899	2.9991
SD	0.0211	0.0674	0.0998
CV	0.0277	0.0452	0.0333
$\overline{CV} = 0.036$			

4.6. Storage data

Samples were generated at 1.5 mg/m³ ethylene oxide at 85% relative humidity, 22°C and 633 mm Hg. All samples were taken for 20 min at 0.05 L/min. Four samples were analyzed as soon as possible (1 day later) and fifteen samples were stored at refrigerated (5°C) and fifteen samples were stored at ambient temperature (23°C). These stored samples were analyzed over a period of nineteen days. The results are shown graphically in Figures 4.6.1. and 4.6.2.

Table 4.6.
Storage Tests

storage time (days)	% recovery (refrigerated)		% recovery (ambient)	
1*	87.0	93.0	94.0	92.0
4	92.0	93.0	91.0	91.0
6	92.0	92.0		
8			92.0	86.0
10	91.7	95.5	95.7	
11			90.0	82.0
13	78.0	81.4	82.4	
14			78.5	72.1
18	66.0	68.0		
19			64.0	77.0

* Results from the first day of storage used in both storage tests.

4.7. Breakthrough data

Breakthrough studies were done at 2 ppm (3.6 mg/m³) at approximately 85% relative humidity and 22°C (ambient temperature). Two charcoal tubes were used in series. The backup tube was changed

every 10 min and analyzed for breakthrough. The flow rate was 0.050 L/min. The results are shown graphically in Figure 4.7.

Table 4.7.
Breakthrough Data

tube no.	time (min)	% breakthrough
1	10	none
2	20	none
3	30	none
4	40	1.23
5	50	3.46
6	60	18.71
7	70	39.2
8	80	53.3
9	90	72.0
10	100	96.0
11	110	113.0
12	120	133.9

The 5% breakthrough volume (2.6 L) was reached after 52 min of sampling.

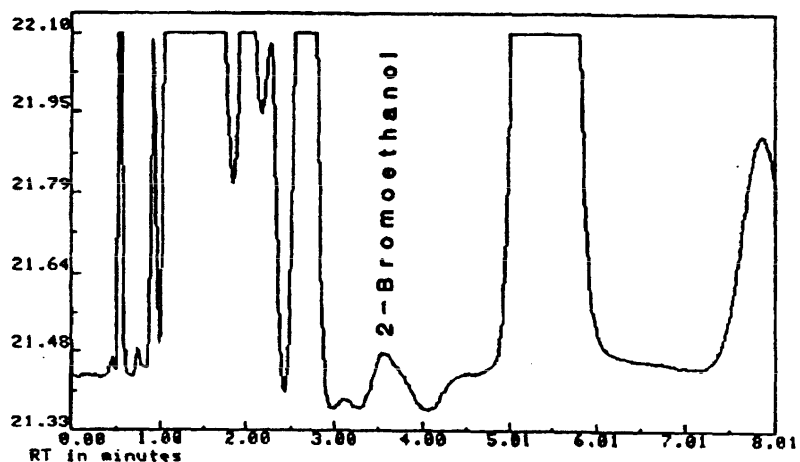


Figure 4.1. Chromatogram of the analytical detection limit.

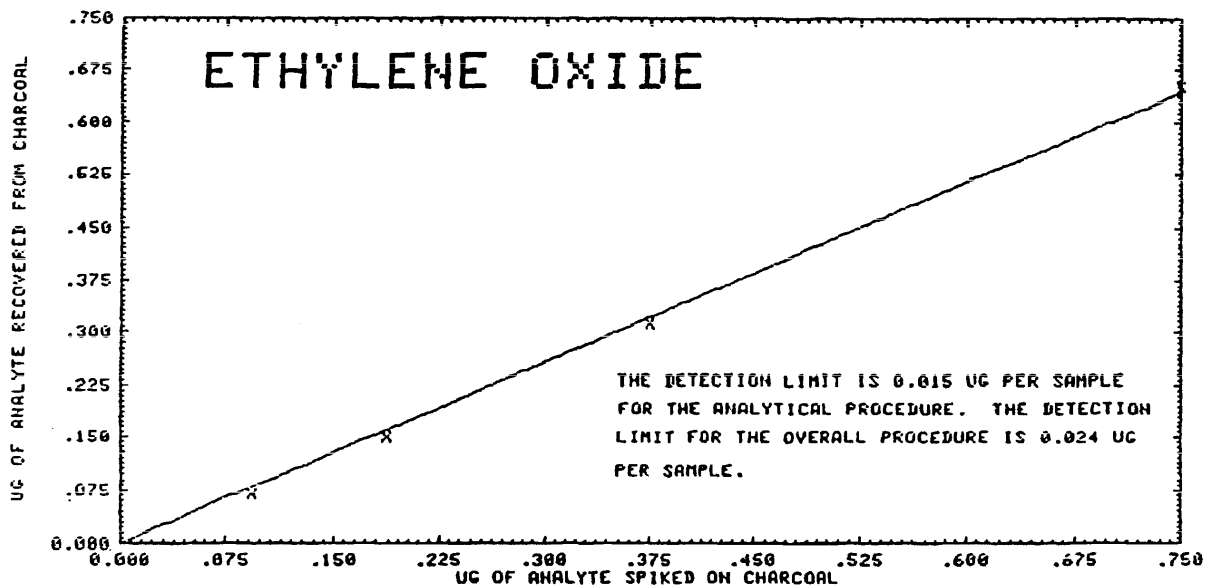


Figure 4.2.1. Determination of the overall detection limit.

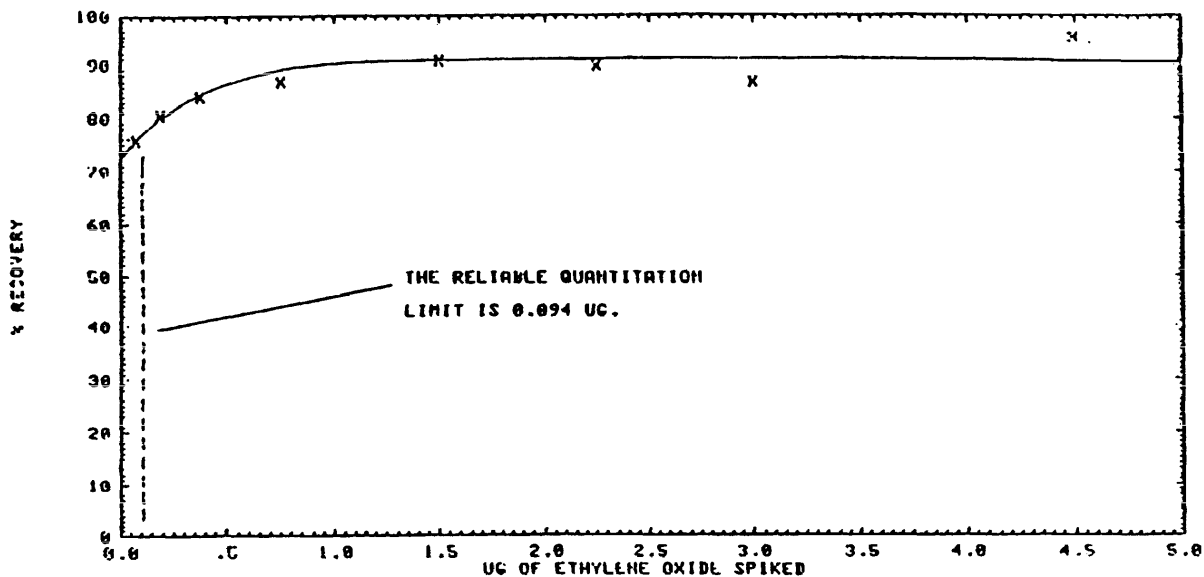


Figure 4.2.2. Reliable quantitation limit.

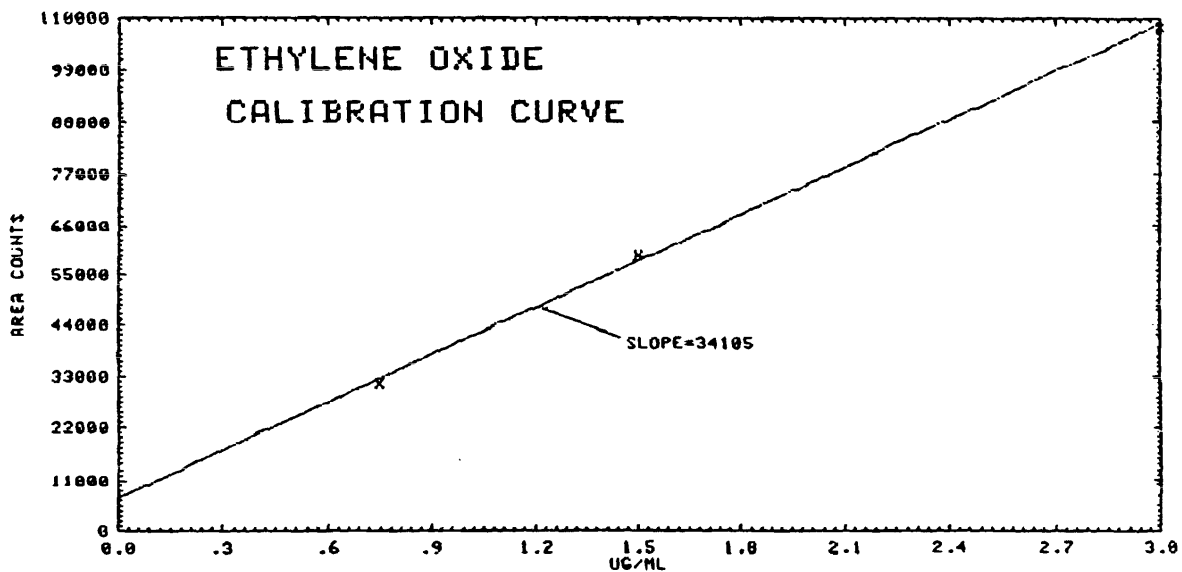


Figure 4.3. Calibration curve.

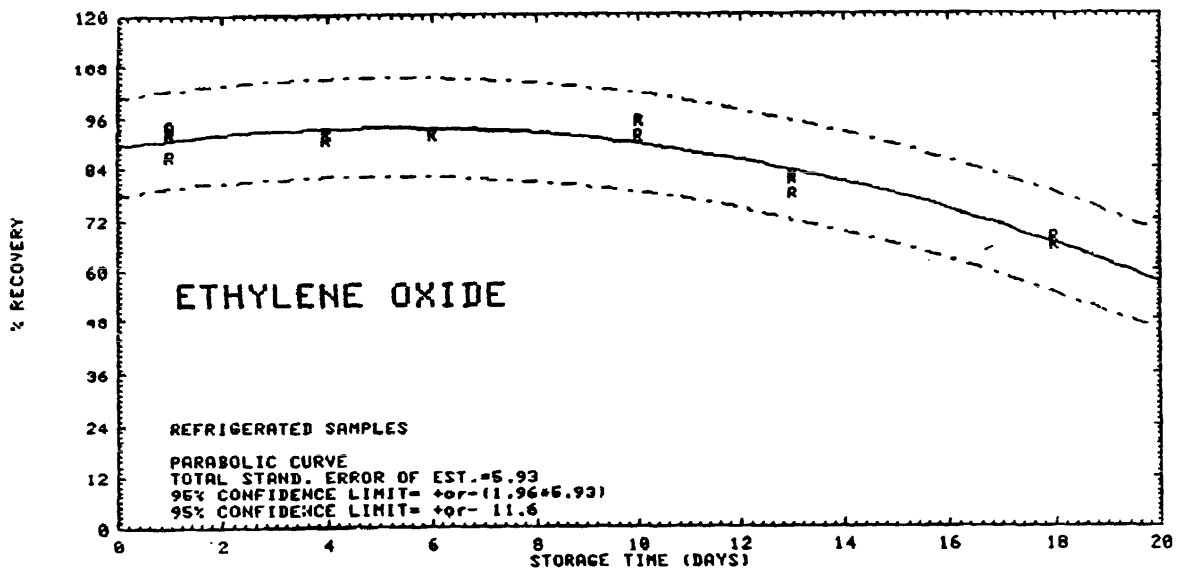


Figure 4.6.1. Refrigerated storage.

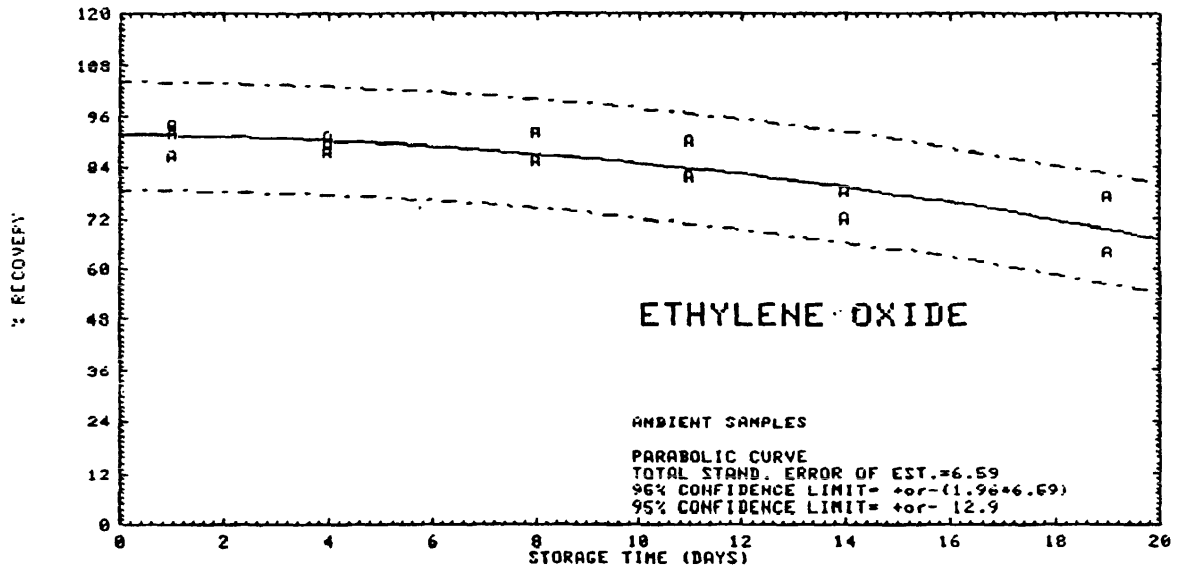


Figure 4.6.2. Ambient storage.

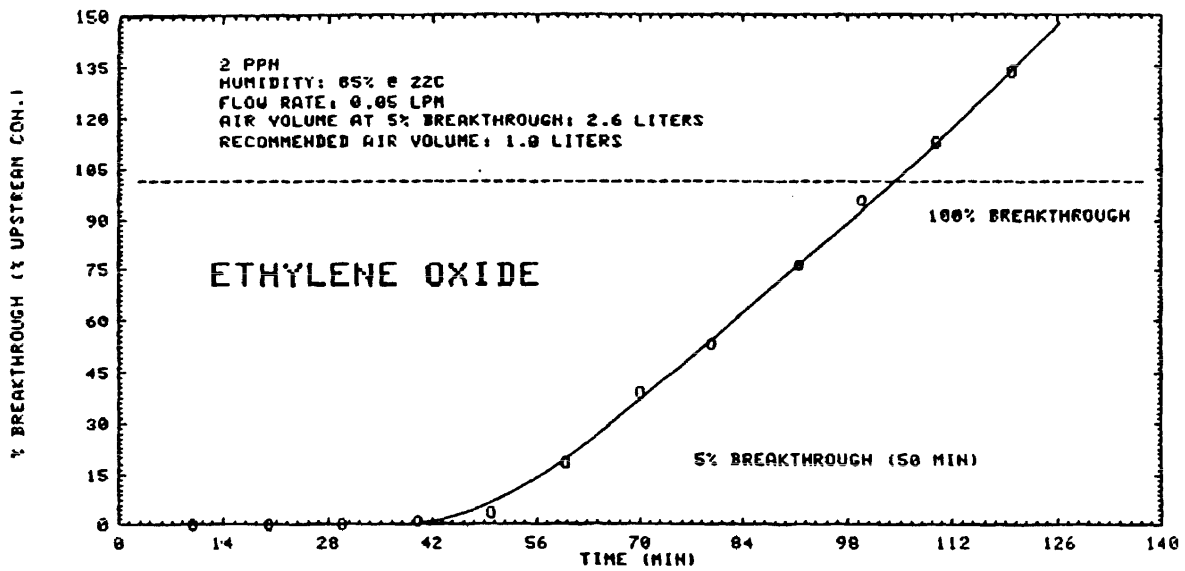


Figure 4.7. Breakthrough curve.

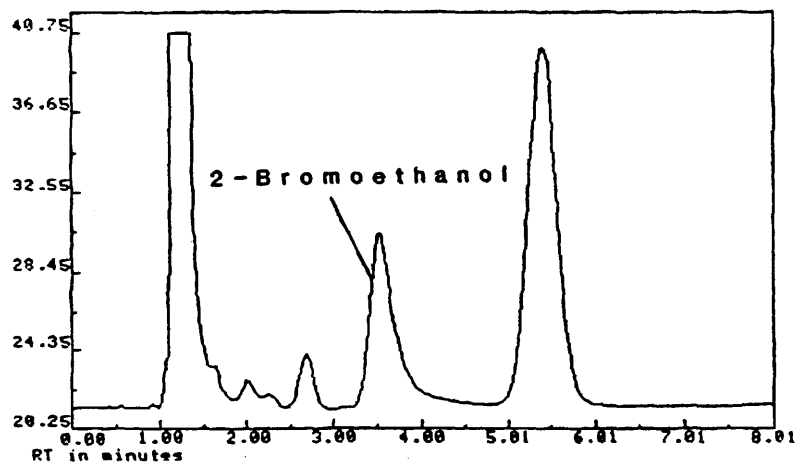


Figure 4.8. Chromatogram of a standard.

5. References

- 5.1. "NIOSH Manual of Analytical Methods", 2nd ed. NIOSH: Cincinnati, 1977; Method S286.
- 5.2. Hine, C.H., and Rowe, V.K. In "Industrial Hygiene and Toxicology", 2nd ed.; Patty, F.A., Fassett, D.W., and Irish, D.D., Eds.; Interscience Publishers: New York, 1963; Vol. II, p. 1627.
- 5.3. "Current Intelligence Bulletin 33: Ethylene Oxide" NIOSH, May 1981.
- 5.4. "IARC Monographs on the Evaluation of Carcinogenic Risk of Chemicals to Man", International Agency for Research on Cancer: Lyon, 1976; Vol. II, p. 157.
- 5.5. Sax, N. I. "Dangerous Properties of Industrial Materials", 4th ed.; Van Nostrand Reinhold Company. New York, 1975; p. 741.
- 5.6. "The Condensed Chemical Dictionary", 9th ed.; Hawley, G.G., ed.; Van Nostrand Reinhold Company, New York, 1977; p. 361.