

CYCLOHEXANONE



---

Method no.: 01

Matrix: Air

Target concentration: 50 ppm (200 mg/m<sup>3</sup>) (OSHA PEL)

Procedure: Collection of vapors on Chromosorb 106, desorption with carbon disulfide, analysis by gas chromatography with flame ionization detection.

Detection limit based on recommended air volume: 0.05 ppm  
(For analytical procedure only)

Recommended air volume and sampling rate: 10 L at 0.05 to 0.2 L/min

Standard error of estimate at the target concentration: 5.2%  
(Section 4.3)

Status of Method: Evaluated method. This method has been subjected to the established evaluation procedures of the Organic Methods Evaluation Branch.

Date: April 1979

Chemist: Carl J. Elskamp

Organic Methods Evaluation Branch  
OSHA Analytical Laboratory  
Salt Lake City, Utah

## 1. General Discussion

### 1.1 Background

#### 1.1.1 History

In the past, cyclohexanone has been determined by collection on activated charcoal, desorption with carbon disulfide and analysis by gas chromatography (Ref. 5.1). It has now been found that once cyclohexanone is collected on charcoal, the recovery drops off severely with time (Ref. 5.2). This new method requires collection of cyclohexanone vapors on Chromosorb 106 (Ref. 5.3) instead of charcoal. The cyclohexanone on Chromosorb 106 remains stable for at least 16 days, even at room temperature. The OSHA Analytical Laboratory, Salt Lake City, Utah, has analyzed from 400 to 500 cyclohexanone samples per year for the last two years.

#### 1.1.2 Toxic effects (This section is for information only and should not be taken as the basis of OSHA policy)

Breathing vapors constitute the prime route of absorption by the body. The most important effects of inhalation of concentrations exceeding the PEL (50 ppm, 200 mg/m<sup>3</sup>) are eye, nose, and throat irritation and narcosis (Ref. 5.4 and 5.5). It can cause a dermatitis upon skin contact and also can cause damage to the liver and kidneys (Ref. 5.6). A concentration of 75 ppm inhaled by a human was considered an irritant (Ref. 5.7).

#### 1.1.3 Operations where exposures occur

The most important use for cyclohexanone is a chemical intermediate in the production of adipic acid (Ref. 5.4). It is also used as a solvent for cellulose esters and ethers, dyes, resins, lacquers, shellac, oil, and fats. Its properties make it desirable as a degreaser, a spotting agent for removing stains in the dry cleaning and textile industries, a solvent in paint removers and printing inks, and in the plastics industry (Ref. 5.5).

#### 1.1.4 Size of work population that face exposure - unknown.

#### 1.1.5 Physical properties (Ref. 5.4)

CAS number:	108-94-1
molecular weight:	98.14
boiling point:	155.6°C
specific gravity:	0.9478 at 20°C/4°C
flash point:	111°F (43.6°C) Closed Cup 129°F (54°C) Open Cup
lower explosive limit:	1.1%
evaporation rate (ether = 1):	22.2
color:	colorless to pale yellow
odor:	ketone-type odor, similar to acetone and peppermint
other names:	pimelic ketone, cyclohexyl ketone, ketohexamethylene, Anone, Hytrol O, Nadone, Sextone

structural formula:



### 1.2 Detection limit, precision, sensitivity, and working range

1.2.1 The detection limit for the analytical procedure is 0.8 ng. The coefficient of variation at this level is 1.17%. This is equivalent to 0.05 ppm for a 10-L air sample based on a 0.4- $\mu$ L injection. (Section 4.1)

1.2.2 The pooled coefficient of variation for 1 to 4 mg of cyclohexanone per sample is 0.33% for the analytical method. This range is equivalent to 25 to 100 ppm cyclohexanone for a 10-L air sample. (Section 4.2)

1.2.3 The sensitivity of the analytical procedure over a concentration range representing 0.5 to 2 times the PEL based on the recommended air volume is 396,000 area counts per mg/mL. The sensitivity is determined by the slope of the calibration curve. The sensitivity

will vary somewhat with the particular instrumentation and parameters used in the analysis. (Section 4.2)

- 1.2.4 The lower limit of the estimated working range, assuming adequate desorption efficiency, is 1 ppm. The upper limit of the working range is dependent on the capacity of the Chromosorb 106.

### 1.3 Accuracy

- 1.3.1 The overall procedure must provide results that are at least  $\pm 25\%$  of the true values at the 95% confidence interval.
- 1.3.2 The recovery of analyte from the collection medium must be 75% or greater.
- 1.3.3 The method meets the required criteria at the PEL concentration for a 16-day sample storage period. (Section 4.3)

### 1.4 Advantages

- 1.4.1 The sampling procedure is convenient.
- 1.4.2 The analytical procedure is quick, sensitive and reproducible.
- 1.4.3 Reanalysis of samples is possible.
- 1.4.4 Samples are stable, even at room temperature.
- 1.4.5 It may be possible to analyze other compounds simultaneously.
- 1.4.6 Interferences can be circumvented by proper selection of GC parameters.

### 1.5 Disadvantages

Some interfering compounds are extracted from untreated Chromosorb 106. (Section 3.6.3)

## 2. Sampling Procedure

### 2.1 Apparatus

- 2.1.1 A personal sampling pump that can be calibrated to within  $\pm 5\%$  of the recommended flow rate with the sampling tube in line.
- 2.1.2 Chromosorb 106 tubes: Glass tube, with both ends heat sealed, 85 mm  $\times$  6-mm o.d.  $\times$  4-mm i.d., containing 100-mg front and 50-mg backup sections of 60/80 mesh Chromosorb 106. SKC No. 226-49-60-106 tubes or equivalent.

### 2.2 Reagents

None required.

### 2.3 Sampling technique

- 2.3.1 Immediately before sampling, break open the ends of the Chromosorb 106 tube. All tubes must be from the same lot.
- 2.3.2 Connect the Chromosorb 106 tube to the sampling pump with flexible tubing. The short section of the Chromosorb 106 tube is used as a backup and should be positioned nearer the sampling pump.
- 2.3.3 The tube should be placed in a vertical position during sampling to minimize channeling.
- 2.3.4 Air being sampled should not pass through any hose or tubing before entering the Chromosorb 106 tube.
- 2.3.5 Seal the Chromosorb 106 tube with plastic caps immediately after sampling.

- 2.3.6 With each batch of samples, submit at least one blank tube from the same lot used for samples. This tube should be subjected to exactly the same handling as samples (break, seal, transport) except that no air is drawn through it.
- 2.3.7 Transport the samples (and corresponding paperwork) to the lab for analysis.
- 2.3.8 If bulk samples are submitted for analysis, they should be transported in glass containers with Teflon-lined caps. These samples must not be put in the same container used for the Chromosorb 106 tubes.

## 2.4 Breakthrough

The average breakthrough (5% breakthrough) volume for three separate samples from a 100-ppm cyclohexanone test atmosphere at 80% relative humidity was 12.8 L when sampled at 0.18 L/min.

## 2.5 Desorption efficiency

- 2.5.1 The desorption efficiency, from liquid injections onto the front section of the tubes, averaged 97.7% from 25 to 100 ppm for a 10-L air sample. (Section 4.4)
- 2.5.2 The desorption efficiency of a particular compound may vary from one laboratory to another and also from one batch of Chromosorb 106 to another. Thus, it is necessary to determine the desorption efficiency for a particular batch of Chromosorb 106.

## 2.6 Recommended air volume and sampling rate

- 2.6.1 The recommended air volume is 10 L.
- 2.6.2 The large pressure drops across the Chromosorb 106 tubes limit the maximum flowrate. The acceptable flowrate range is 0.05 to 0.2 L/min.

## 2.7 Interferences

- 2.7.1 It is unknown if any other compound would severely interfere with the collection of cyclohexanone on Chromosorb 106. In general, the presence of other solvents will decrease the breakthrough volume for a particular solvent.
- 2.7.2 Suspected interferences should be listed on the sample data sheets.

## 2.8 Safety precautions

- 2.8.1 Attach the sampling equipment on the employee so that it does not interfere with work performance.
- 2.8.2 Wear safety glasses when breaking the ends of the sampling tubes.
- 2.8.3 Place the sampling tube in a holder so the sharp end is not exposed while sampling.

# 3. Analytical Procedure

## 3.1 Apparatus

- 3.1.1 Gas chromatograph equipped with a flame ionization detector.
- 3.1.2 GC column capable of separating cyclohexanone and an internal standard from any interferences and carbon disulfide. The column used for validation studies was: 10-ft × 1/8-in. stainless steel, 20% SP2100, 0.1% CW 1500 on 100/120 Supelcoport.
- 3.1.3 An electronic integrator or some other suitable method of measuring peak areas.
- 3.1.4 Two-milliliter vials with Teflon-lined caps.
- 3.1.5 Microliter syringes, 10- $\mu$ L or other convenient sizes for preparing standards and 1- $\mu$ L for sample injections.

- 3.1.6 Pipets for dispensing carbon disulfide. The Glenco 1-mL dispenser is adequate and convenient.
- 3.1.7 Volumetric flasks, 5-mL and other convenient sizes for preparing standards.
- 3.2 Reagents
- 3.2.1 Cyclohexanone, reagent grade.
- 3.2.2 Chromatographic grade carbon disulfide.
- 3.2.3 A reagent grade internal standard, such as ethyl benzene.
- 3.2.4 Desorbing reagent - 1  $\mu$ L internal standard/1 mL CS<sub>2</sub>.
- 3.2.5 Purified GC grade helium, hydrogen, and air.
- 3.3 Sample preparation
- 3.3.1 The front and back sections of each sample are transferred to separate 2-mL vials.
- 3.3.2 Each section is desorbed with 1.0 mL of desorbing reagent.
- 3.3.3 The vials are sealed immediately and allowed to desorb for 30 min with intermittent shaking.
- 3.4 Standard preparation
- 3.4.1 Standards are prepared by diluting the pure cyclohexanone with the desorbing reagent.
- 3.4.2 A concentration of 1  $\mu$ L of cyclohexanone per 1 mL of desorbing reagent equals 26.28 ppm for a 10-L air sample desorbed with 1 mL. This amount is uncorrected for desorption efficiency.
- 3.5 Analysis
- 3.5.1 GC conditions
- |                                     |                        |
|-------------------------------------|------------------------|
| flow rates (mL/min)                 | zone temperatures (°C) |
| helium: 25                          | injector: 200          |
| hydrogen: 35                        | detector: 250          |
| air: 250                            | column: 125            |
| injection size: 1 $\mu$ L           |                        |
| cyclohexanone elution time: 5.7 min |                        |
- 3.5.2 Peak areas are measured by an integrator or other suitable means.
- 3.5.3 An internal standard procedure is used. The integrator is calibrated to report results in ppm for a 10-L air sample after correction for desorption efficiency.
- 3.6 Interferences
- 3.6.1 Any compound eluting in the same general time as cyclohexanone or the internal standard is a potential interference. Possible interferences are listed on the sample data sheets. GC parameters should be chosen so these interferences will pose no problems.
- 3.6.2 GC parameters may be changed to circumvent most interferences.
- 3.6.3 When Chromosorb 106 is desorbed with CS<sub>2</sub>, some late eluting peaks appear on the chromatograms. These do not interfere with the analysis but the analysis time is increased. It may be possible to pretreat the Chromosorb 106 by heating it under a flow of an inert gas or by extracting it with a solvent prior to preparing the tubes for sampling.
- 3.6.4 Retention time data on a single column is not considered proof of chemical identity. Samples over the PEL should be confirmed by GC/MS or other suitable means.

### 3.7 Calculations

Since the integrator is programmed to report results in ppm for a 10-L air sample (corrected for desorption efficiency), the following calculation is used:

$$\text{ppm cyclohexanone} = \frac{(\text{ppm on report})(10)}{\text{liters of air sampled}}$$

### 3.8 Safety precautions

- 3.8.1 All work done with the solvents (preparation of standards, desorption of samples, etc.) should be done in a hood.
- 3.8.2 Avoid any skin contact with all of the solvents.
- 3.8.3 Wear safety glasses at all times.

## 4. Backup Data

### 4.1 Detection limit

A standard containing 0.002  $\mu\text{L}$  cyclohexanone/mL  $\text{CS}_2$  (1.90  $\mu\text{g}/\text{mL}$ ) was used. Peak heights were used since the integrator could not pick up the peaks.

injection	peak height (mm)	
1	34.5	$\bar{X}=35.0$
2	35.5	SD=0.408
3	35	CV=1.17%
4	35	

GC conditions used for determination of detection limit:

Hewlett-Packard 5840A, flame ionization detector

column: 10-ft  $\times$  1/8-in. stainless steel, 20% SP2100/0.1% CW1500

attenuation: 0

injection size: 0.4  $\mu\text{L}$

temperatures ( $^{\circ}\text{C}$ )                      Flows (mL/min)

injector: 200                                  helium: 24

detector: 200                                 hydrogen: 35

column: 125                                  air: 240

Detection Limit = 1.90  $\text{ng}/\mu\text{L} \times 0.4 \mu\text{L} = 0.8 \text{ ng}$

This amount is equivalent to 0.05 ppm for a 10-L air sample desorbed with 1.0 mL  $\text{CS}_2$ .

### 4.2 Instrument response to the analyte and analytical precision

injection	0.5 $\times$ PEL 948 $\mu\text{g}$	1 $\times$ PEL 1896 $\mu\text{g}$	2 $\times$ PEL 3792 $\mu\text{g}$
1	971	1889	3772
2	966	1897	3781
3	964	1899	3787
4		1891	3775
5	976	190	3787
6	970	1902	3791
$\bar{X}$	969.4	1896.3	3782.2
SD	4.67	5.20	7.49
Cv	0.00482	0.0027	0.0020
CV	0.0033		

See Figure 4.2. for calibration curve.

### 4.3 Storage Study

Samples were collected on Chromosorb 106 sampling tubes at 0.18 L/min for 55 min from a 50-ppm cyclohexanone test atmosphere which had a relative humidity of 80%. Five samples were analyzed immediately and fifteen samples were stored at room temperature (23°C), and fifteen were stored at refrigerator temperature (-5°C). The stored samples were then analyzed on the days indicated. The recoveries listed are not corrected for desorption efficiency.

Table 4.3  
Storage Tests

storage time (days)	% recovery (ambient)			% recovery (refrigerated)		
0	92.4	94.3	93.9	92.4	94.3	93.9
	92.5	93.8		92.5	93.8	
3	93.9	93.7	95.3	93.6	93.7	97.7
6	94.3	93.9	95.2	95.5	93.0	94.8
9	95.0	91.2	92.1	98.8	94.1	90.2
11	93.0	91.3	93.1	93.6	93.2	92.5
16	90.2	89.8	91.6	91.2	91.6	89.7

The standard error of estimate for room temperature samples is 5.2%. This includes a sampling error of ±5%. See Figures 4.3.1, 4.3.2, and 4.3.3.

### 4.4 Desorption efficiency

Table 4.4  
Desorption Efficiency of Cyclohexanone from Chromosorb 106 with Carbon Disulfide

× target concn µg/sample	0.5×	1×	2×
	0.9952	1.990	3.981
desorption efficiency, %	97.2	98.1	96.7
	96.4	98.1	96.9
	98.2	98.1	98.2
	96.5	97.4	97.3
	97.6	100.1	99.1
	96.4	97.9	97.8
$\bar{X}$ mean	97.0	98.3	97.7
	97.7		

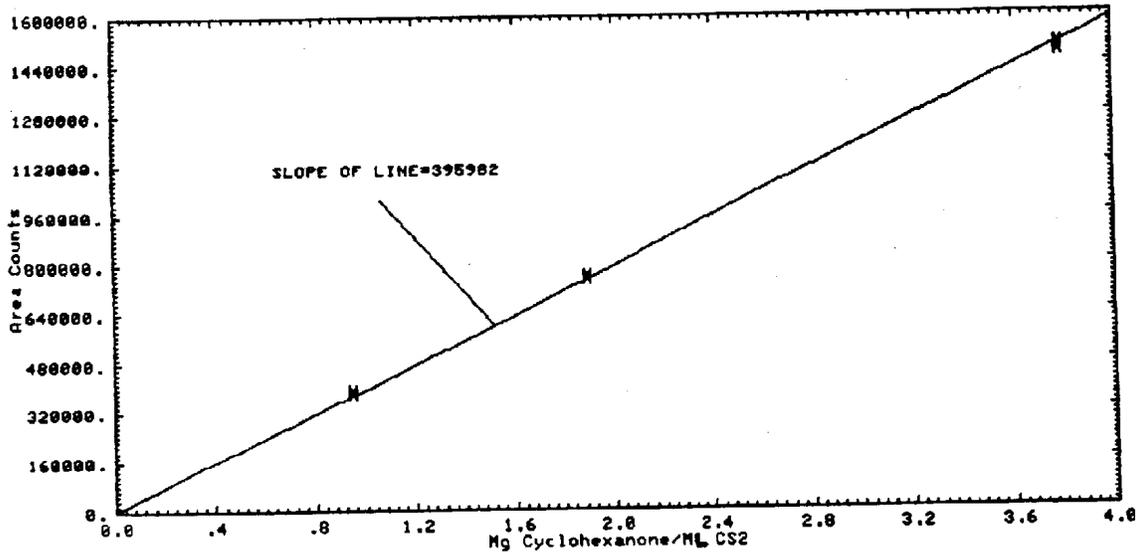


Figure 4.2. Calibration curve.

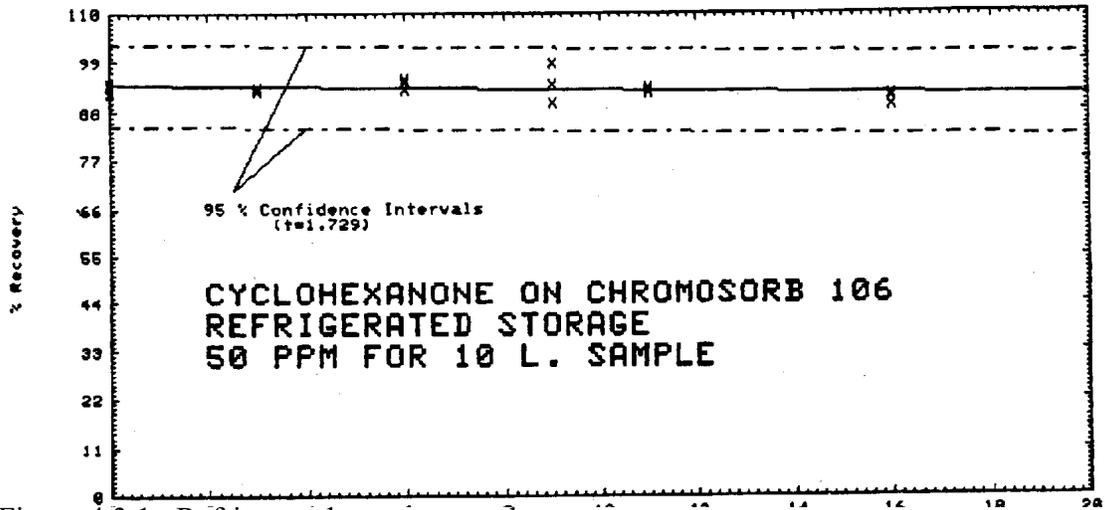


Figure 4.3.1. Refrigerated storage samples.

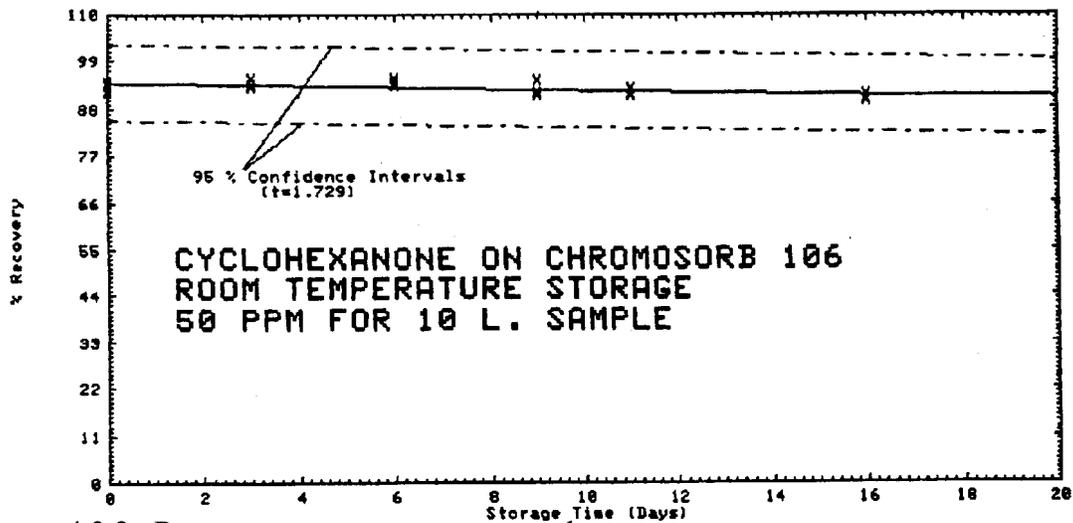


Figure 4.3.2. Room temperature storage samples.

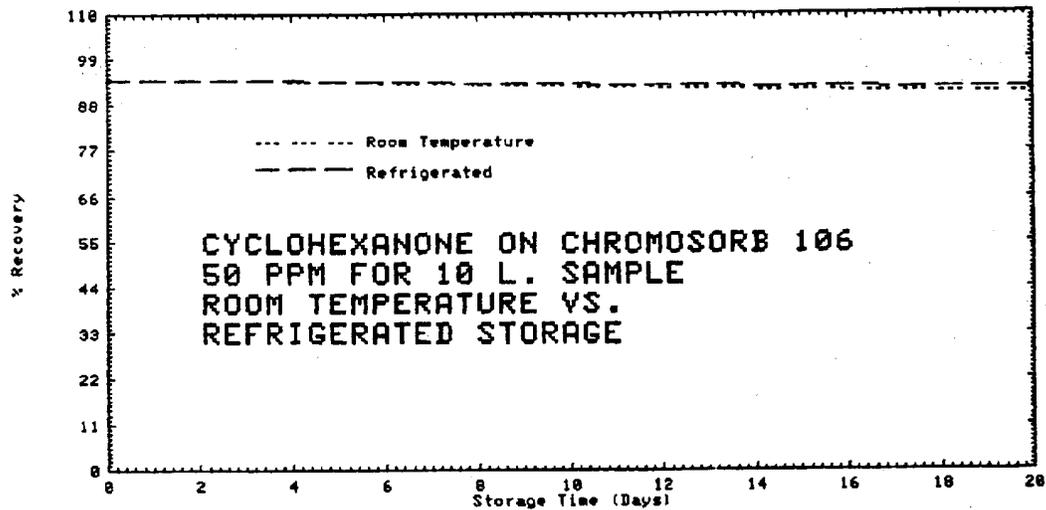


Figure 4.3.3. Room temperature vs. refrigerated storage samples.

## 5. References

- 5.1 "NIOSH Manual of Analytical Methods, 2nd edition", Vol. 2, Method S19.
- 5.2 "An Investigative Report on the Stability of Selected Ketones on Activated Charcoal" by Carl J. Elskamp, OSHA Analytical Lab, Salt lake City, Utah, unpublished.
- 5.3 Chromosorb 106 is a cross-linked polystyrene porous polymer prepared by Johns-Manville Corp.
- 5.4 Hygiene Guide Series: Cyclohexanone, *Am. Ind. Hy. Asso. J.*, 26:630, 1965.
- 5.5 "Industrial Hygiene and Toxicology", 2nd Revised Edition, Volume II, Frank E. Patty, editor, page 1765.
- 5.6 "Dangerous Properties of Industrial Materials", Fourth Edition, W. Irving Sax, p. 591.
- 5.7 "Registry of Toxic Effects of Chemical Substances", 1976 ed., U.S.D.H.E.W., Index Number GW 10500.